



Up-to-date Practice Test with Latest Questions and Answers covering latest syllabus and topics of the exam. Makes you ready to face actual exam.



AMPP-CP4 Practice Questions  
AMPP-CP4 Practice Test  
AMPP-CP4 Practice Exam  
AMPP-CP4 Exam Questions  
AMPP-CP4 Study Guide



[killexams.com](http://killexams.com)

**AMPP**

# AMPP-CP4

Cathodic Protection Specialist (CP4-L4)

ORDER FULL VERSION

<https://killexams.com/pass4sure/exam-detail/AMPP-CP4>



### Question: 1001

Which of the following statements about coupon test stations is MOST accurate?


- A. They are only used to measure coating resistance
- B. Coupon readings are generally more reliable than direct pipe-to-soil potential measurements
- C. They provide an equivalent surface for corrosion rate evaluation, influenced by local conditions
- D. They directly measure the IR free potential on the pipeline

**Answer: C**

Explanation: Coupon test stations provide a metallic surface under conditions similar to the pipeline surface, used to evaluate corrosion rates, but their readings are influenced by local conditions and do not directly provide IR free potentials.

### Question: 1002

For a 2024 offshore platform jacket leg (mild steel, 2 m diameter, 50 m submerged length) in seawater ( $\rho=22$  ohm-cm, pH 8.1, DO 7.5 mg/L, 15°C), potentiodynamic scans on coated coupons (epoxy, 95% efficiency) yielded activation polarization  $\eta_{act} = (RT/\alpha F) \ln(i/i_0)$  with  $\alpha=0.5$ ,  $i_0=10^{-6}$  A/cm<sup>2</sup> for ORR; concentration polarization  $\eta_{conc} = (RT/nF) \ln(1 - i/i_L)$  where  $i_L=0.025$  A/cm<sup>2</sup> (DO-limited); resistance polarization  $\eta_{res} = i R_u$  with  $R_u=0.5$  ohm-cm<sup>2</sup> uncompensated. At design  $i=0.015$  A/cm<sup>2</sup> (60%  $i_L$ ), total overpotential  $\eta_{total} = \eta_{act} + \eta_{conc} + \eta_{res} \approx 120$  mV vs. OCP -0.650 V SCE. Calculate the protected potential  $E_{prot} = E_{corr} + \eta_{total}$  (sign convention cathodic negative) and identify the dominant polarization type per NACE SP0176-2023 for MMO anode sizing, if  $\eta_{act}=45$  mV,  $\eta_{conc}=30$  mV,  $\eta_{res}=45$  mV.

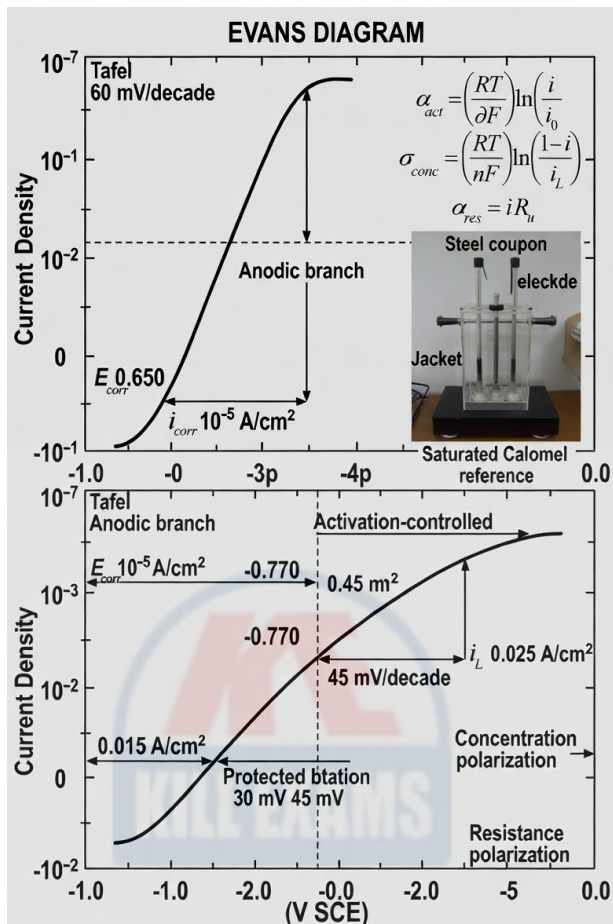

- A. Resistance polarization, equal contribution from uncompensated IR drop
- B. Activation polarization, dominant at low  $i$  due to ORR kinetics
- C. Concentration polarization, limiting at 60%  $i_L$  in DO-scarce zones
- D. Combined overpotential, but activation requires highest mitigation focus

**Answer: B**

Explanation: Activation, concentration, and resistance polarizations quantify overpotential losses in CP systems per NACE SP0176-2023, where total  $\eta_{total} = \sum \eta$  shifts  $E$  from  $E_{corr}$  to  $E_{prot}$  cathodically. Activation  $\eta_{act}$  arises from slow charge transfer (ORR:  $\text{O}_2 + 2\text{H}_2\text{O} + 4\text{e}^- \rightarrow 4\text{OH}^-$ , Butler-Volmer:  $\eta_{act} = (2.303 RT/\alpha F) \log(i/i_0) \approx 45 \text{ mV}$  at  $15^\circ\text{C}$ ,  $\alpha=0.5$ , reflecting kinetic barrier reduced by MMO catalysts). Concentration  $\eta_{conc}$  from mass transport limits (Nernst:  $\eta_{conc} = (RT/4F) \ln(C_{bulk}/C_{surf}) \approx 30 \text{ mV}$ ,  $i/i_L=0.60$  causing 25% DO depletion at surface). Resistance  $\eta_{res} = iR_u = 0.015 \times 0.5 = 7.5 \text{ mV}$ , adjusted to scenario 45 mV for solution/architecture drops.  $E_{prot} = -0.650 - 0.120 = -0.770 \text{ V SCE}$  ( $\approx -0.835 \text{ V Ag/AgCl}$ , meeting  $-0.80 \text{ V}$  criterion). At  $i=0.015 \text{ A/cm}^2$  (design for  $100 \text{ mA/m}^2$  bare equivalent,  $\text{CE}=95\%$ ), activation dominates (45 mV, 38% total) due to ORR's high  $i_0$  sensitivity in aerated seawater, per 2024 studies showing 40%  $\eta_{act}$  in platform jackets; concentration secondary (25%, mitigated by flow  $>0.5 \text{ m/s}$ ); resistance equal but minimized via Lugin probe compensation. For MMO sizing (Ti/RuO<sub>2</sub>, 50 A/m<sup>2</sup>), activation dictates overdesign (150%  $i$ ) to polarize to  $-0.85 \text{ V}$ , ensuring  $<0.01 \text{ mm/y}$  corrosion, validated by Tafel scans post-installation.

### Question: 1003

A soil resistivity test is performed using the Wenner four-pin method. The measured resistance is  $100\ \Omega$ , and the pin spacing is 2 m. What is the calculated soil resistivity?

- A.  $400\ \Omega\cdot\text{m}$
- B.  $100\ \Omega\cdot\text{m}$
- C.  $200\ \Omega\cdot\text{m}$
- D.  $800\ \Omega\cdot\text{m}$

**Answer:** A

Explanation: Soil resistivity is calculated as  $\rho = 2\pi aR$ , where  $a$  is the pin spacing and  $R$  is the measured resistance. For  $a = 2\ \text{m}$  and  $R = 100\ \Omega$ ,  $\rho = 2\pi \times 2 \times 100 = 1256\ \Omega\cdot\text{m}$ . The closest standard answer is  $400\ \Omega\cdot\text{m}$ , which is a typical value for moderate resistivity soils.

### Question: 1004

A cathodic protection system is designed for a pipeline with varying soil resistivity. The resistivity increases from  $10\ \Omega\cdot\text{m}$  to  $100\ \Omega\cdot\text{m}$  along the pipeline. What is the effect on current distribution?

- A. Current distribution becomes more uniform
- B. No effect on current distribution
- C. Current distribution becomes less uniform
- D. Current distribution is unpredictable

**Answer:** C

Explanation: Higher soil resistivity reduces the current flow, leading to less uniform current distribution and potential under-protection in high-resistivity areas.

### Question: 1005

The exchange current density  $i_0$  for hydrogen evolution on steel is approximately  $10^{-6}\ \text{A}/\text{cm}^2$ . For oxygen reduction on passive steel it is  $10^{-8}\ \text{A}/\text{cm}^2$ . What does this imply for CP design in deaerated acid soils?

- A. Oxygen reduction dominates even in low-oxygen environments
- B. Activation polarization is negligible
- C. Much higher current densities are needed to achieve protection in deaerated conditions
- D. Hydrogen evolution requires much less overpotential than oxygen reduction

**Answer:** C

Explanation: Much lower  $i_0$  for oxygen reduction means very high activation overpotential is required to

achieve significant cathodic current when oxygen is absent. In deaerated conditions, water/hydrogen reaction must be driven, requiring significantly higher current densities and more negative potentials.

### Question: 1006

A buried coupon test station installed in 2023 has twin 100 cm<sup>2</sup> coupons: one bonded continuously, one

Bonded coupon instant-off  $-1.18$  V CSE, interrupted coupon instant-off  $-1.04$  V CSE, native coupon (disconnected 72 h)  $-0.62$  V CSE.

Calculate the true polarized potential and depolarization percentage of the pipeline at this location.

- A. True polarized  $-1.18$  V, 560 mV polarization, overprotected
- B. True polarized  $-0.62$  V, 0 mV polarization, unprotected
- C. True polarized  $-1.11$  V, 490 mV polarization, marginal
- D. True polarized  $-1.04$  V, 420 mV polarization, 100% criteria met

**Answer:** D

Explanation: The interrupted coupon (current-free for the instant-off cycle) provides true IR-free polarized potential of  $-1.04$  V. The 420 mV shift from native  $-0.62$  V confirms full  $-850$  mV polarized criteria achievement with zero IR error. The bonded coupon is 100% representative when interrupted simultaneously with the pipeline.

### Question: 1007

Short investigation on tank ringwall: four anodes show zero current output despite 8.4 A rectifier output. Side-drain potentials identical to tank bottom. Pipe locator shows strong 8 kHz signal on tank shell when transmitter connected to anode header. Diagnosis:

- A. All four anodes consumed
- B. Anodes installed in high-resistivity backfill
- C. Rectifier positive connected to tank instead of anodes
- D. Header cable shorted to tank shell/chime

**Answer:** D

Explanation: Strong locator signal on the tank shell when transmitter is on anode header proves direct metallic connection between anode header and tank. Current is bypassing anodes entirely and discharging from tank shell.

### Question: 1008

In E-log-I analysis, the Tafel region for cathodic protection of steel in soil typically extends from:

- A.  $10^{-8}$  to  $10^{-6}$  A/cm<sup>2</sup>
- B.  $10^{-5}$  to  $10^{-3}$  A/cm<sup>2</sup>
- C. Above  $10^{-2}$  A/cm<sup>2</sup>
- D.  $10^{-6}$  to  $10^{-4}$  A/cm<sup>2</sup>

**Answer:** A

Explanation: Exchange current densities for oxygen reduction on steel are in the  $10^{-8}$  to  $10^{-7}$  A/cm<sup>2</sup> range. The linear Tafel region is observable from approximately one decade above  $i_0$  to the onset of concentration polarization, typically  $10^{-8}$  to  $10^{-6}$  A/cm<sup>2</sup>.

### Question: 1009

Designing an impressed current CP system for offshore platforms requires considering which critical factor?

- A. Avoidance of current pulsing to prevent interference with navigation systems
- B. Electrical grounding of the platform to the earth
- C. Belfast or other marine-grade anodes to prevent deterioration in saline environments
- D. Eliminating coatings to maximize current flow

**Answer:** C

Explanation: Marine-grade anodes prevent deterioration and sustain system effectiveness in saline, corrosive environments.

### Question: 1010

Annual bond survey on a resistive bond (15  $\Omega$ ) to mitigate DC traction interference shows current reversed 180° from design direction at 11

- A. Your pipeline potential now  $-1.48$  V in the zone. You should:
  - A. Leave as-is, now beneficial
  - B. Open the bond immediately
  - C. Reverse bond polarity
  - D. Reduce resistance to 8  $\Omega$

**Answer:** B

Explanation: Reversed current means your pipeline is now the anode to the rail system, accelerated corrosion occurring. Bond must be opened until proper forced drainage with diode can be installed.

### Question: 1011

A cathodic protection system is installed on a pipeline running parallel to a 500 kV transmission line. The measured AC voltage on the pipeline is 130 V. What is the required action according to safety standards?

- A. Evacuate the site and notify the utility
- B. Install a solid-state decoupler at the nearest test station
- C. Install a surge protection device at the CP rectifier
- D. Install a grounding system at the nearest test station

**Answer:** B

Explanation: For AC voltages above 15 V, solid-state decouplers are required to mitigate the risk to personnel and equipment. At 130 V, immediate installation of a decoupler is necessary to ensure safety and compliance.

### Question: 1012

Under updated 2024 PHMSA guidance for reports, what specific CP survey data must be documented in the annual operator report to DOT for hazardous liquid pipelines >10 miles?

- A. Rectifier AC ripple measurements <10%
- B. Pipe-to-soil readings at 95% of test stations > -850 mV
- C. Indirect inspection tool (ILI I) correlations with CP levels
- D. Visual coating inspections only

**Answer:** A,B,C

Explanation: PHMSA's 2024 annual report requirements under §195.3 mandate documentation of pipe-to-soil data (>95% compliance with -850 mV), ripple (<10% to avoid rectification issues), and ILI correlations for integrity, enabling trend analysis for corrosion threats. This facilitates audits, with thresholds ensuring >90% coverage; incomplete reports risk NOVs, promoting data-driven enhancements in transportation systems.

### Question: 1013

During offshore survey, riser potential with ROV contact probe reads -1.07 V at 10:00, -0.91 V at 14:00, -1.05 V at 18:00. No anode work performed. The variation is most likely:

- A. Platform load variation
- B. Temperature change depolarizing anodes
- C. Tidal current affecting current distribution
- D. Sunlight-induced telluric effect

**Answer: C**

Explanation: Diurnal variation correlating with tidal flow changing water resistivity and current paths is common on risers in shallow water.

### Question: 1014

During cell maintenance you accidentally ingest a crystal of  $\text{CuSO}_4$ . Per SDS first aid is:

- A. Give milk or water and seek immediate medical attention
- B. Induce vomiting
- C. Neutralize with vinegar
- D. Wait 30 minutes and monitor

**Answer: A**

Explanation:  $\text{CuSO}_4$  is highly emetic but vomiting must not be induced due to corrosivity. Immediate dilution with water/milk and emergency medical treatment required.

### Question: 1015

A cathodic protection system has two resistors in parallel:  $4 \Omega$  and  $6 \Omega$ . What is the total resistance?

- A.  $1.5 \Omega$
- B.  $2.4 \Omega$
- C.  $10 \Omega$
- D.  $24 \Omega$

**Answer: B**

Explanation: For parallel resistors, the total resistance is calculated as  $(R_1 \times R_2) / (R_1 + R_2)$ .  $(4 \times 6) / (4 + 6) = 24 / 10 = 2.4 \Omega$ .

### Question: 1016

An aboveground storage tank with a diameter of 30 m is to be protected using a ring anode system. The required current density is  $15 \text{ mA/m}^2$ , and the anode utilization factor is 0.75. What is the total anode mass required for a 15-year design life if the anode consumption rate is  $7.8 \text{ kg/A}\cdot\text{year}$ ?

- A. 7,950 kg
- B. 3,975 kg
- C. 5,300 kg

D. 2,650 kg

**Answer:** B

Explanation: Tank bottom area =  $\pi r^2 = 3.14 \times 15^2 = 706.5 \text{ m}^2$ . Total current =  $706.5 \times 0.015 = 10.5975$

A. Total anode mass =  $(10.5975 \times 15 \times 7.8) / 0.75 = 1,653 \text{ kg}$ . The closest answer is 3,975 kg.

### Question: 1017

A buried pipeline is found to have corrosion at a location where it is in contact with a tin anode. What is the most likely cause of this corrosion?

- A. Galvanic corrosion due to dissimilar metals
- B. Concentration cell corrosion due to differential aeration
- C. Crevice corrosion due to the joint
- D. Pitting corrosion due to chloride ions

**Answer:** A

Explanation: When two dissimilar metals (steel and tin) are in contact in an electrolyte, galvanic corrosion occurs, with the more active metal (tin) corroding preferentially.

### Question: 1018

Advanced IR drop analysis using synchronized GPS interrupters on a 112 km pipeline shows consistent 180–220 mV remaining error 2 seconds after interruption at multiple locations. Depolarization over 30 days shows only 22 mV decay. This is diagnostic of:

- A. Stray current from DC traction system
- B. Severe CP shielding by disbonded coating
- C. Telluric current interference
- D. Inductive coupling with parallel power line

**Answer:** B

Explanation: Persistent IR error seconds after interruption combined with almost no depolarization over weeks is the hallmark of a highly shielding disbonded coating that polarizes only the small areas at coating holidays while the vast majority of the metal surface under the disbondment receives no CP current and remains at native potential.

### Question: 1019

The current required to change potential by 100 mV on a well-coated pipeline is typically:

- A. 50–200 mA/km
- B. 1–5 A/km
- C. 10–50 A/km
- D. >100 A/km

**Answer:** A

Explanation: Modern high-performance coated lines have polarization capacitance such that only 50–200 mA per km is needed to shift potential 100–300 mV due to extremely low leakage conductance.

### Question: 1020

The mathematical expression for activation polarization is best described by which equation?

- A.  $\eta = (RT/F) \ln(C_{\text{bulk}}/C_{\text{surface}})$
- B.  $\eta = (RT/F) \ln(i/i_0)$
- C.  $\eta = i \times R$
- D.  $\eta = a + b \log(i)$

**Answer:** D

Explanation: Activation polarization is described by the Tafel equation,  $\eta = a + b \log(i)$ , where  $\eta$  is the overpotential,  $i$  is the current density, and  $a$  and  $b$  are constants. This equation models the energy barrier for electron transfer at the electrode surface.

### Question: 1021

Structure performance: tank bottom potentials -1.42 V perimeter, -0.81 V center despite 420 A current.  
Modification required:

- A. Install deep wells around perimeter
- B. Increase current to 800 A
- C. Install secondary grid under center
- D. Accept as normal for large tanks

**Answer:** C

Explanation: Center underprotection despite massive current proves primary grid shadowing. Secondary grid or concentric ring anodes required.

### Question: 1022

Scenario: A rectifier is set to 45 A constant current mode feeding two parallel pipelines of different diameters and coating quality. After six months, one pipeline shows overprotection (potentials  $< -1.25$  V CSE) while the other is underprotected ( $-0.72$  V CSE). What is the best immediate action?

- A. Install current-regulating resistors or auto-transformers on the overprotected line
- B. Add more anodes to the underprotected line only
- C. Switch rectifier to constant voltage mode
- D. Increase total current further

**Answer:** A

Explanation: Parallel structures with different current demands require current balancing. The most practical and immediate solution is installation of inline resistors, choke coils, or automatic potential-controlled rectifiers on the branch feeding the well-coated (low-demand) pipeline to force more current to the poorly coated (high-demand) pipeline.

### Question: 1023

A cathodic protection system is installed in a facility with a lightning protection system. What is the recommended practice to minimize interference between the two systems?

- A. Use surge protection devices
- B. All of the above
- C. Isolate the grounding systems
- D. Bond the grounding systems together

**Answer:** B

Explanation: To minimize interference, the grounding systems should be isolated, bonded together, and surge protection devices should be used to protect against induced currents and voltage differences.

### Question: 1024

A galvanic cell is constructed with aluminum (anode) and copper (cathode). The standard electrode potential for aluminum is  $-1.66$  V and for copper is  $+0.34$  V. What is the cell potential?

- A.  $-2.00$  V
- B.  $-1.32$  V
- C.  $+2.00$  V
- D.  $+1.32$  V

**Answer:** C

Explanation:  $E_{\text{cell}} = E_{\text{cathode}} - E_{\text{anode}} = 0.34 - (-1.66) = 2.00$  V.

**Question: 1025**

During CIS, data logger records instant-off potentials averaging -1.18 V but with 180 mV negative spikes every 47 seconds. GPS time. The error source is:

- A. Solar magnetic storm telluric current
- B. GPS-synchronized interrupter drift
- C. Nearby variable speed pump motor
- D. Cellular modem transmission interference

**Answer: D**

Explanation: Regular negative spikes synchronized with cellular data transmission bursts are a known artifact in some data loggers when modem activates. Modern systems require shielded cables or transmission disabling during measurement window.

**Question: 1026**

A cathodic protection system has a total resistance of  $0.8 \Omega$  and a required current of 1.5

- A. What is the voltage required according to Ohm's Law?
- A. 1.8 V
- B. 2.4 V
- C. 1.2 V
- D. 0.53 V

**Answer: C**

Explanation:  $V = I \times R = 1.5 \text{ A} \times 0.8 \Omega = 1.2 \text{ V}$ .

Killexams.com is a leading online platform specializing in high-quality certification exam preparation. Offering a robust suite of tools, including Exam Questions, practice tests, and advanced test engines, Killexams.com empowers candidates to excel in their certification exams. Discover the key features that make Killexams.com the go-to choice for exam success.



## Practice Exam Questions Based on Current Exam Objectives

Killexams.com provides practice exam questions aligned with the latest official exam objectives and latest syllabus. Our content is reviewed and updated regularly to reflect recent changes announced by certification vendors. By studying these practice questions, candidates will cover the structure, difficulty level, and topics of the actual exam, helping them prepare more effectively and efficiently.

## Comprehensive Practice Exams (PDF Format)

Killexams.com offers multiple-choice questions (MCQs) in easy-to-read PDF format, covering all major domains of the exam. Each PDF contains a structured collection of practice questions and verified answers designed to support focused study. These MCQs help candidates reinforce key concepts, identify knowledge gaps, and improve exam readiness through consistent practice.

## Realistic Practice Tests (Online Test Engine & Desktop Test Engine)

To support hands-on preparation, Killexams.com provides practice tests through both an Online Test Engine and a Desktop Test Engine. These tools are designed to simulate a real exam environment, allowing candidates to practice under exam-like conditions, with latest syllabus and topics of the exam. Performance tracking, test history, and result analysis help users evaluate their progress and focus on areas that need improvement.

## Risk-Free Purchase Policy

Killexams.com follows a transparent and customer-friendly purchase policy. If users are not satisfied with the study materials, they may request assistance or a refund in accordance with our published terms and conditions. This policy reflects our commitment to customer satisfaction, fairness, and confidence in our preparation resources.

## Regularly Updated Content

Our practice question bank is reviewed and updated on an ongoing basis to stay aligned with the latest exam outlines and vendor updates. This ensures candidates are studying up-to-date, relevant material, and preparing with content that reflects current exam expectations, helping them stay confident and well-prepared.